

SPECIFICATIONS

Model	TonoVue
Intraocular Pressure	
Measurement range	1– 60 mmHg
Measurement range setting	Auto/ 30 mmHg/ 60 mmHg
Measurement principle	Air puff method
Display units	mmHg/hpa
Working distance	11 mm
Alignment	Fully automatic 3D tracking
Chinrest	Motorized
Display	10.1" LCD touch screen
Printer	Thermal line printer with auto cutter
Interface	USB / RS232
Power supply	AC100V to 240V, 50/60Hz, auto selected
Operating Environment	Temperature: 10°C to 35°C Humidity: 30% to 90%
Dimensions (WxDxH)	282 mm x 500 mm x 500 mm
Weight	17 Kg

TonoVue


Fully Automated Non-Contact
Tonometer



3D Tracking



Measurement



Soft Air Puff



Touch Screen



Auto Cutter



All Done by Single Tap

With fully automatic 3D tracking technique, multiple IOP measurements can be done by single tap on the screen. Simply click 'Start', the examination will begin and the result will be printed out directly.



TonoVue		
Patient ID:		
Operator ID:		
No. :		
Time:		

IOP		mmHg

	Right	Left
	15	17
	16	16
	15	16

Avg.	15.3	16.3
C. IOP	16.3	15.3

Crystalvue Medical Corp.		

Patient Friendly- Soft and Fast

The Automatic Air Puff Control System controls the amount of air required for each individual eye. It provides softer and quieter air puff, which makes patient feel less uncomfortable. With intelligent 3D tracking, the measurements can be done fast and precisely. It shortens exam time, which not only simplifies the examination process for doctors and nurses, but also reduces the discomfort or strains for patients.

User Friendly- Simple and Clear

The large 10.1" screen and touch panel is easy to control. The instruction and icons are clear and straightforward, making it simple and easy for anyone to operate. There are also more than 10 built-in languages for users to select.




Connectivity

TonoVue® has built in the software of patient management (database). This software enables easy and fast access to patient data through touch panel, USB or RS232.

Thermal Printer with Auto Cutter

The measurements can be printed out automatically by thermal printer, and then be nicely cut by the auto cutter.

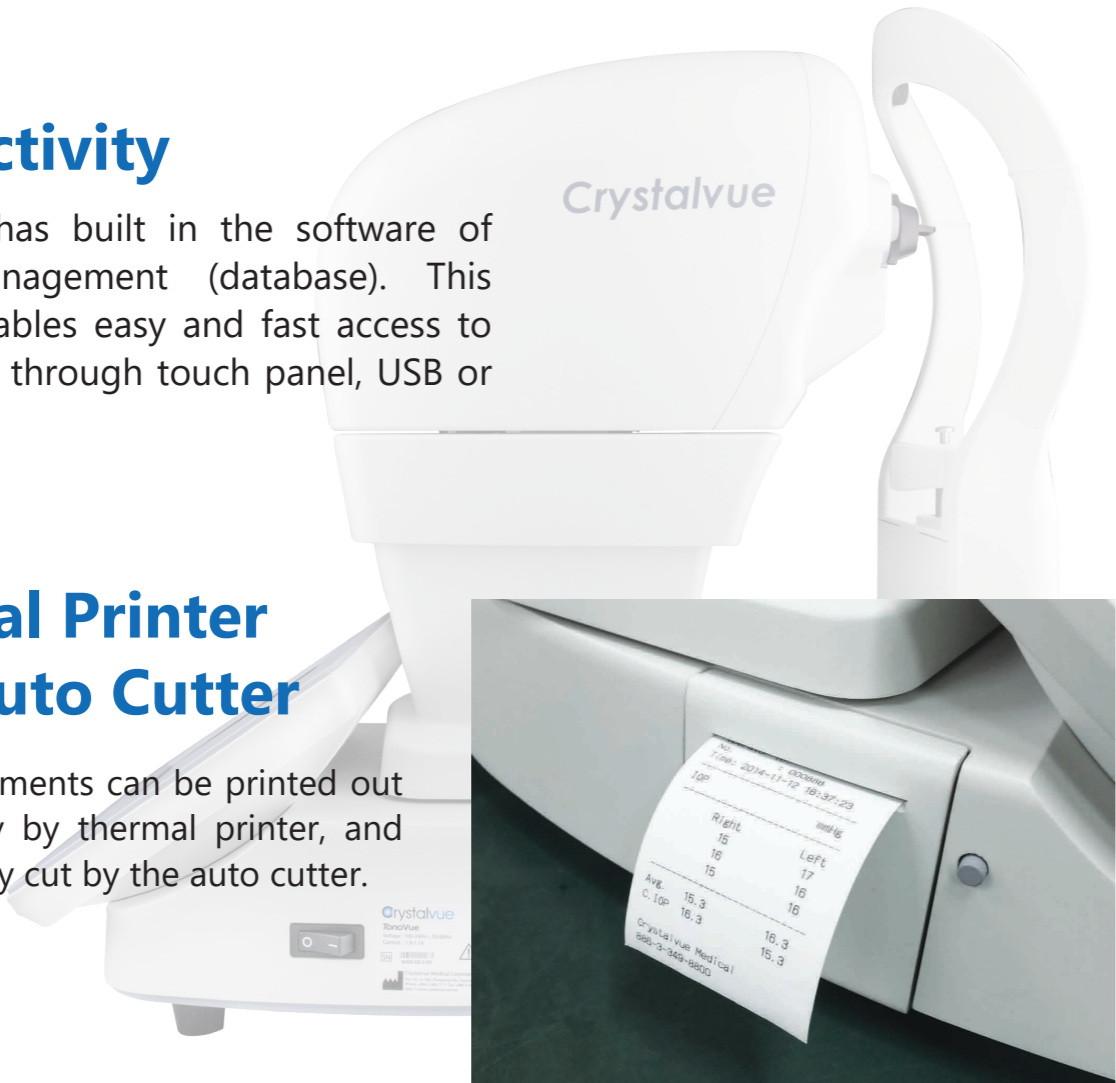

Calculation of Compensated IOP

The studies show that the central corneal thickness (CCT) could affect the accuracy of IOP measurement. For example, thinner corneas contribute to underestimation of IOP value. TonoVue® provides compensated IOP values by inputting the CCT values. The compensated IOP formula can also be customized by user.

